


# QC Test

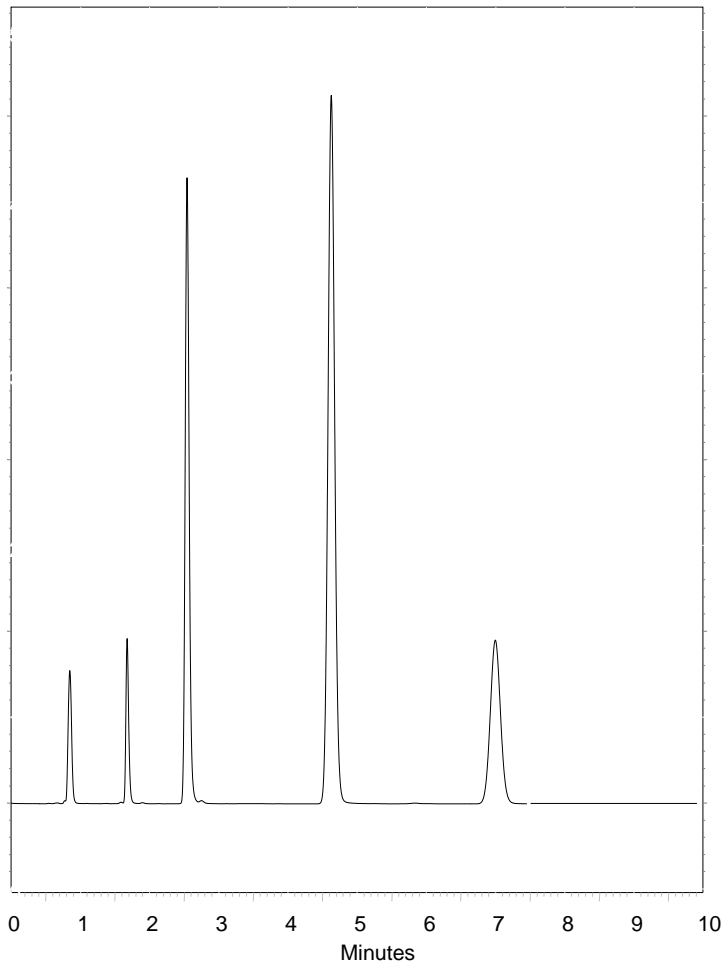

Column : **Fortis C18**  
**100x4.6mm 5 $\mu$**

p/n : **F18-050505**

Mobile Phase: **40/60 Water/ACN**

Flow : **1.0ml/min**

Temp : **25°C**

$\lambda$  : **254nm**

- 1. Uracil**
- 2. Phenol**
- 3. 4-Ethylaniline**
- 4. N,N-Dimethylaniline**
- 5. Naphthalene**